SIEMENS

Siemens Remote Services

CO

Hardware Installation Guide

Telerad+SRS Router 1720 ISDN

Partnumber 75 57 346
Partnumber 75 57 338 (IPSEC)

© Siemens AG 2002
The reproduction, transmission or use of this document or its contents is not permitted without express written authority. Offenders will be liable for damages. All rights, including rights created by patent grant or registration of a utility model or design, are reserved.

Print No.: COIT-000.812.10.01.02
Replaces: n.a.

English
Doc. Gen. Date: 02-02

Revision history

Chapter	Pages	Revision
all	all	01

1. UNPACK THE BOX 4

2. BEFORE INSTALLATION 4

3. CONNECTING POWER AND TURNING THE ROUTER ON 5

4. CONNECTING CISCO 1720 TO THE LAN 6

5. CONNECTING CISCO 1720 TO THE WAN / ISDN 7

6. CONNECTING THE CONSOLE PORT 8

7. CONFIGURE PC (E.G. HYPERTERMINAL) FOR COMMUNICATION 9

8. CONFIGURING GLOBAL PARAMETERS 11

9. FINAL CONFIGURATION 12

10. APPENDIX 13

1. Unpack the Box

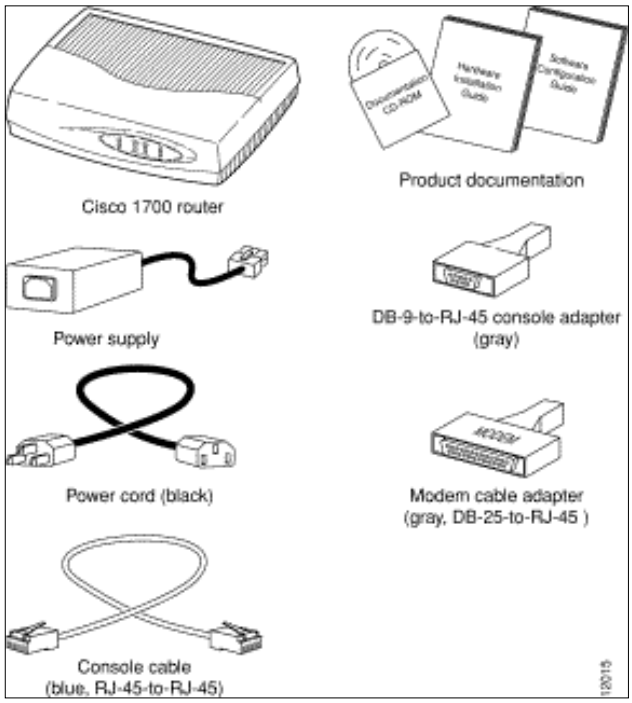

2. Before Installation

Cisco 1700 series routers are shipped to you ready for desktop mounting. Before connecting the router to the network and power supply, simply set the router on a desktop, shelf, or other flat surface. The router you got is preconfigured by SIEMENS Medical Solutions. The router package includes power cords for the US and Europe. You need to provide a power cord for other countries. Pay attention to the Maximum Cable Lengths (see Appendix E).

ISDN BRI Line Configuration Requirements
Before using a Cisco 1700 series router with an ISDN BRI you must order two correctly configured ISDN BRI lines from your local telecommunications service provider.
This process varies significantly from provider to provider on a national and international basis. However, following are some general guidelines:

- Ask for two channels to be called by one number.
- Ask for delivery of calling line identification. This is also known as *Caller ID* or *Automatic Number Identification* (ANI).
- Ask for a point-to-multipoint service **data** line (subaddressing is required).
- Ask for a Network Terminator (NT). You need ISDN BRI **S/T** lines.

ISDN on an internal PABX (Private Automatic Branch eXchange) is not recommended. Also refer to the SRS Planning Guide. If you are familiar with the hardware installation and the configuration connection to your PC, go to chapter 8.

For the configuration of the router you will have to know what the following paramters of your ISDN connection are:

- The **ISDN switch type** and in some cases
- The **spid numbers**

Your ISDN service provider will be able to tell you what these parameters are.

3. Connecting Power and Turning the Router On

You can verify your installation by checking the appropriate LEDs during the installation process if you switch the router on before making any network connections.

Follow these steps to connect the router to the power supply and turn it on:

Step 1 Connect the DC power cable (included with the router) from the power supply to the DC power input on the rear panel of the router. (Figure 1)
Step 2 Connect the female end of the cable to the male receptacle of the power supply.
Step 3 Connect the male end of the power cable to the power outlet.
Step 4 On the rear panel of the router, turn the power ON by setting the switch labeled I / O to the I position.
Step 5 Check the following LEDs:

- The PWR LED (Front Panel)---On if power is being supplied to router.
- The OK LED (Front Panel)---On while router software is operational. (This LED first blinks and then remains on continuously.)
- The OK LED (Rear Panel, next to Flash PC card slot)---On if the Flash memory card is installed correctly.

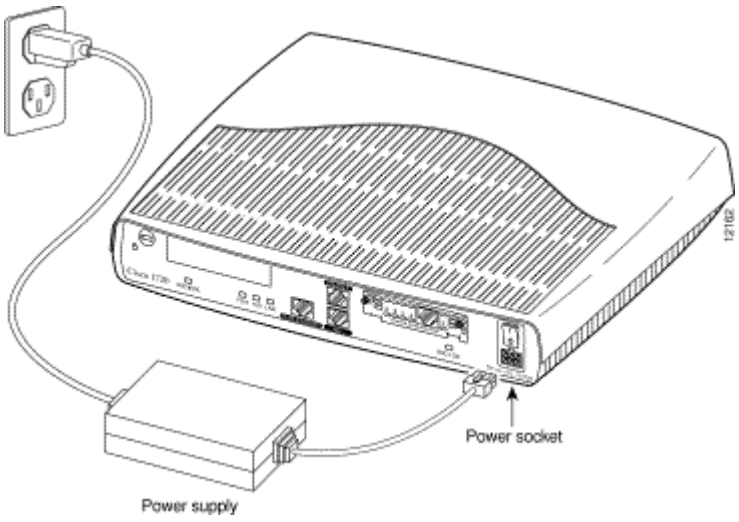

Figure 1

4. Connecting Cisco 1720 to the LAN

One of the gray straight-through RJ-45-to-RJ-45 cables (contained in the package – do not use a cable with the label „CAB-U-RJ45“) is necessary for this connection. Follow these steps to connect the router to a 10|100BaseTX Ethernet LAN (Figure 2):

Step 1 Connect one end of the Ethernet cable to the 10|100BaseTX port.
Step 2 Connect the other end of the cable to one of the ports on the 10|100BaseTX hub, switch or network walljack.
Step 3 Check the following LEDs:

- LNK LED (Rear Panel, next to 10|100BaseTX port)---On if the router is connected correctly to the 10|100BaseTX Ethernet LAN.
- ETH ACT LED (Front Panel)---On while there is traffic on the Ethernet LAN.

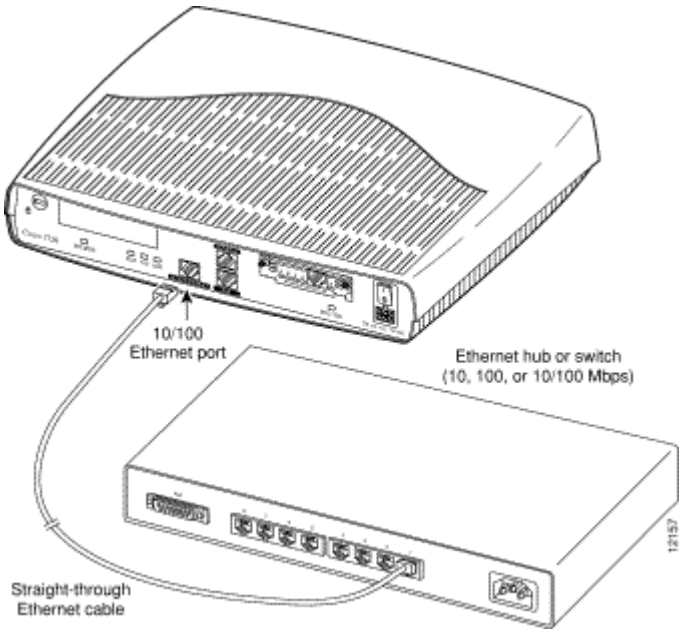

Figure 2

Note: If you want to connect the router directly to a PC, Server, Workstation you will need a cross over RJ-45-to-RJ-45 cable (*not included in the package).*

5. Connecting Cisco 1720 to the WAN / ISDN

The ISDN Service Provider must provide a Network Termination 1 (NT1) device for each of the ISDN interfaces. Two ISDN BRI S/T lines from your Service Provider are necessary. One of the lines will be used for the teleradiology connection, the other one for SIEMENS Remote Service. Use a gray straight-through RJ-45-to-RJ-45 cable for these connections (contained in the package – do not use a cable with the label „CAB-U-RJ45“).

Depending on where the Cisco 1720 is used, the ISDN BRI connection may be different. Follow these steps to connect the Cisco 1720 to the WAN:

Step 1 Use one of the gray RJ-45-to-RJ-45 cables and connect one end of the cable to the ISDN port of the WICØ slot of the router. This will be the port used for the teleradiology connection (Figure 3).

Step 2 Connect the other end of the cable to that NT that belongs to the number ISDN 1 (also marked as teleradiology number in the configuration sheet). *Do not connect ISDN equipment other than the preconfigured router to the same ISDN line (S_0 Bus).*

Step 3 Repeat steps one and two for the ISDN port of the WIC1 slot of the router. It should be connected to the NT with the number ISDN 2, used for SIEMENS Remote Service (in the configuration sheet also marked as SRS number).

Step 4 Check the following LEDs

- The OK LEDs on the rear panel (directly to the right of the ISDN BRI ports) light up once the ISDN port has synchronized with the central office switch.
- The external NT1 might have a LED indicating synchronization with the central office switch or other NT1 status. Check the NT1 documentation.

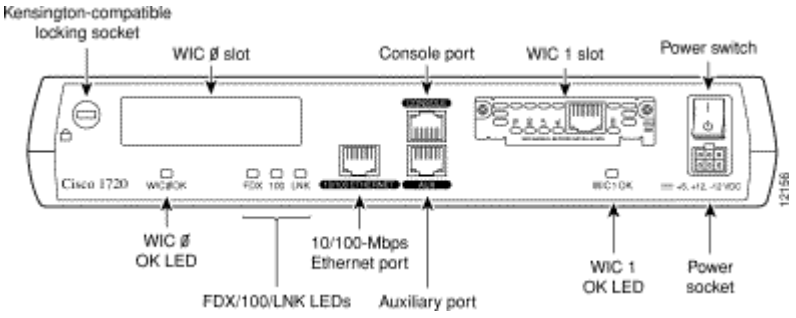

Figure 3

6. Connecting the Console Port

The cable and adapters required for this connection are included in the package. Follow these steps to connect the router to a terminal or PC:

Step 1 Connect one end of the light-blue console cable to the light-blue CONSOLE port of the router (Figure 4).

Step 2 Use the correct adapter to connect the other end of the cable to your terminal or PC (serial interface).

Note If your terminal or PC has a console port that does not match any of the adapters, you must provide the correct adapter for that port.

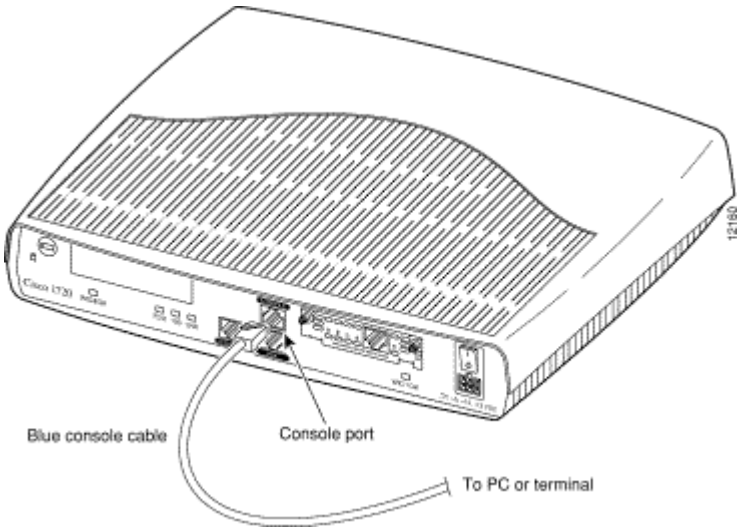

Figure 4

7. Configure PC (e.g. Hyperterminal) for communication

Once your router is correctly connected to your PC, you can start building your configuration. The Windows Hyperterminal emulation is the interface to your Cisco 1720 router.

Step 1 Start Hyperterminal from the „Programs – Accessories – Hyperterminal“ menu in the start panel. If you do not find the program there or anywhere else on your computer, you will have to install it first.

Step 2 In the „Connection Description“ dialogue box

- enter a name for the connection and choose an icon. If you want to save the connection settings, click „OK“
- *or* click „Cancel“

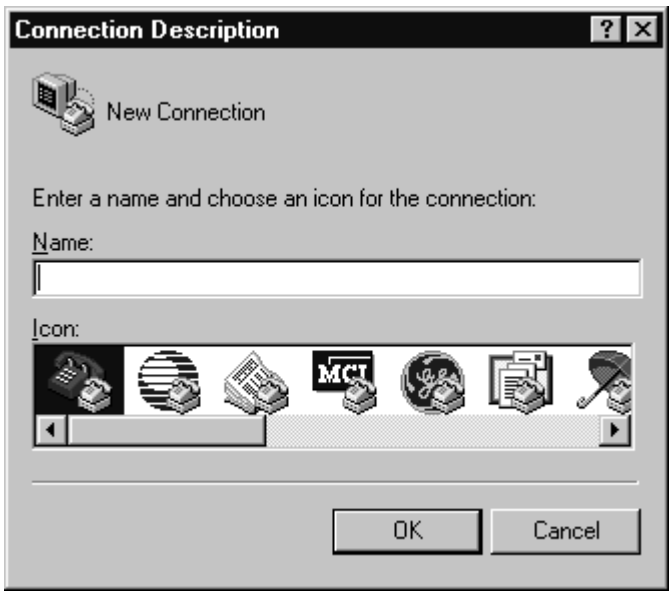

Step 3 Choose „Properties“ from the „File“ menu. On the „Connect to“ tab, check, if the port to which your router is connected (e.g. COM1) is selected.

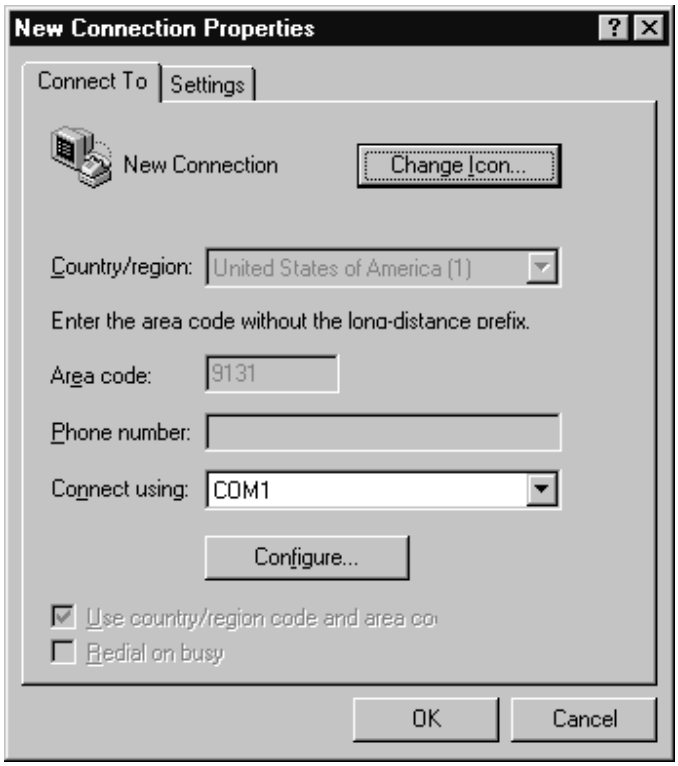

Step 4 Click „Configure“ and make sure that the settings have the following values: Bits per second: 9600, Data bits: 8, Stop bits: 1, Flow control: Hardware. Click „OK“ twice to leave configuration mode.

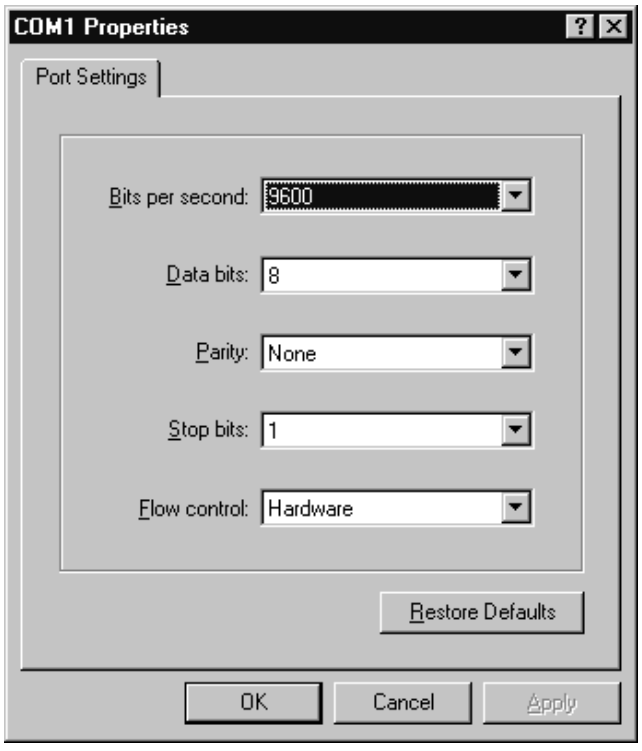

Step 5 Choose „Connect“ from the „Call“ menu to establish a connection to the router.

8. Configuring Global Parameters

The preconfigured router uses the ISDN switch type EURO-ISDN (basic-net3) for Europe. The following steps are necessary *only* if you use another ISDN switch type. Ask your ISDN service provider.

Use the table below to configure some global parameters of the router, including the ISDN switch type the router is connected to by the ISDN line. The switch type also needs to be set for the specific interfaces, e.g. the BRI 0 and 1. The router's name (in front of the prompt), should be a combination of serial number and part number (e.g. jac0356823Qc346).

	Description	Prompt	Command
Step 1	Enter enable mode	JAC0356323Qc346>	**enable** Password: **presec**
Step 2	Enter configuration mode.	JAC0356323Qc346#	**configure terminal**
Step 3	Configure the type of central office switch being used on the ISDN interface. Use the keyword that matches the ISDN switch type that you are using. The PRECONFIGURED router is configured for **basic-net3.** Ask your isdn service provider	JAC0356323Qc346 (config)#	**isdn switch-type** <switch type code> – *[refer to* Appendix C*]*
Step 4	Enter interface BRI 0 mode	JAC0356323Qc346 (config)#	**interface bri 0**
Step 5	Configure the type of central office switch being used on the BRI 0 interface. Use the keyword that matches the ISDN switch type that you are using.	JAC0356323Qc346 (config-if)#	**isdn switch-type** <switch type code> – *[refer to* Appendix C*]*
Step 6	Configure SPID only for switch **basic-5ess, basic-dms100, basic-ni1.** Ask your isdn service provider.	JAC0356323Qc346 (config-if)#	**isdn spid1** <spid-number> **isdn spid2** <spid-number> *[refer to* Appendix D*]*
Step 7	Go back to config mode	JAC0356323Qc346 (config-if)#	**exit**
Step 8	Enter interface BRI 1 mode	JAC0356323Qc346 (config)#	**interface bri 1**
Step 9	Repeat Steps 5 – 7 for BRI 1		<same as steps 5 – 7>
Step 10	Go back to enable mode	JAC0356323Qc346 (config)#	**exit**
Step 11	Save the configuration in the router's memory	JAC0356323Qc346#	**write memory**
Step 12	Display the saved configuration parameters	JAC0356323Qc346#	**show conf**

Note: The router is not preconfigured by SIEMENS Medical Solutions if the prompt says „Router"!

9. Final Configuration – performed by SIEMENS Remote Services

The router hardware configuration is finished. The final configuration will be carried out by SIEMENS Remote Services. **DO NOT** start to configure the router by yourself**!**
In order to use the central service of remote final configuration, fill out the checklist which can be found either in the router box or in the internet at the following address:

`http://sgk.med.siemens.de/access/Telerad/Checklist/Telerad_SRS.doc`

It is important that you do not undertake any additional configurations on your own. The configuration needs to comply with certain security standards known to SRS.

The final configuration includes registering the medical systems by the remote diagnostic server at SIEMENS Remote Services.

10. Appendix

Appendix A) Front Panel LEDs

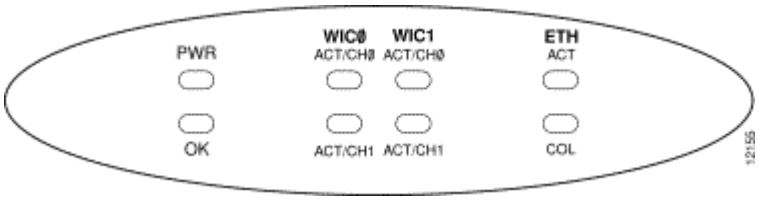

LED	Color	Description
PWR	Green	The router is turned on, and DC power is being supplied.
OK	Green	The router has successfully booted. Blinks during the boot cycle.
ETH ACT	Green	Blinks when there is network activity on the Ethernet port.
ETH COL	Yellow	Blinks when there are packet collisions on the local Ethernet network.
BRI 0 B1	Green	An ISDN connection on B-channel 1.Cisco 1604 only---If an ISDN device connected to the ISDN S/T port is using B-channel 1, the LED turns on.
BRI 0 B2	Green	An ISDN connection on B-channel 2.Cisco 1604 only---If an ISDN device connected to the ISDN S/T port is using B-channel 2, the LED turns on.
WICØ ACT/CHØ	Green	Serial and DSU/CSU cards—Blinks when data is being sent to or received from the port on the card in the WICØ slot. ISDN cards—On solid when the first ISDN B channel is up for the card in the WICØ slot. 2-port serial cards—Blinks when there is data being sent to or received from the first port on the 2-port card in the WICØ slot.
WICØ ACT/CH1	Green	Serial and CSU/DSU cards—Remains off. ISDN cards—On solid when the second ISDN B channel is up for the card in the WICØ slot 2-port serial cards—Blinks when there is data being sent to or received from the second port on the 2-port card in the WICØ slot.
WIC1 ACT/CHØ	Green	Serial and DSU/CSU cards—Blinks when data is being sent to or received from the port on the card in the WIC1 slot. ISDN cards—On solid when the first ISDN B channel is up for the card in the WIC1 slot. 2-port serial cards—Blinks when there is data being sent to or received from the first port on the 2-port card in the WIC1 slot.
WIC1 ACT/CH1	Green	Serial and DSU/CSU cards—Remains off. ISDN cards—On solid when the second ISDN B channel is up for the card in the WIC1 slot. 2-port serial cards—Blinks when there is data being sent to or received from the second port on the 2-port card in the WIC1 slot.

Appendix B) Rear Panel LEDs

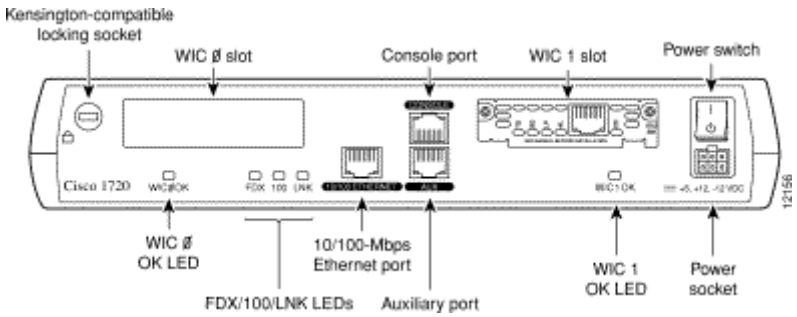

LED	Color	Description
LNK	Green	Indicates 10BaseT link integrity. This LED is not on when connected to an Ethernet network through the AUI port. The Cisco 1605 has two LNK LEDs, one for each Ethernet 10BaseT port.
FDX	Green	On solid—Ethernet port is operating in full-duplex mode. Off—Ethernet port is operating in half-duplex mode
100	Green	On solid—Ethernet port is operating at 100 Mbps. Off—Ethernet port is operating at 10 Mbps.
WICØ OK	Green	On when a WAN interface card is correctly inserted in the card slot
WIC1 OK	Green	On when a WAN interface card is correctly inserted in the card slot.

Appendix C) ISDN BRI Switch Types

ISDN BRI supports a variety of service provider switches. The following table lists, by geographic areas, the ISDN switch types supported by the Cisco 1600 series routers ISDN BRI interface. When configuring the router, use the **isdn switch-type** command followed by the corresponding code.

COUNTRY	SWITCH TYPE CODE
Australia	
Australian TS013 switches	**basic-ts013**
Europe	
Norway NET3 switches (phase 1)	**basic-nwnet3**
NET3 ISDN switches (Germany, UK and others)	**basic-net3**
French VN2 ISDN switches	**vn2**
French VN3 ISDN switches	**vn3**
Japan	
Japanese NTT ISDN switches	**ntt**
North America	
AT&T basic rate switches	**basic-5ess**
NT DMS-100 basic rate switches	**basic-dms100**
National ISDN-1 switches	**basic-ni1**
New Zealand	
New Zealand Net3 switches	**basic-nznet3**

Appendix D) Defining ISDN Service Profile Identifiers

An ISDN service provider, usually a telephone company, can offer a variety of services. Many providers use service profile identifiers (SPIDs) to identify the device that is using the ISDN service, similar to the way that the telephone company uses a telephone number to identify your standard telephone service. If you use a service provider that requires SPIDs, the provider assigns your ISDN device one or more SPIDs when you first subscribe to the service. Providers use different numbering schemes, but a SPID is usually a seven-digit telephone number, plus some optional numbers. The provider also assigns your device one or two local directory numbers (LDNs), which function as the router telephone numbers. The LDN is the number that a remote router dials to make a call to the router.

Note SPIDs have significance only at the local-access ISDN interface. The remote router is assigned a SPID when the ISDN BRI services are ordered for that router.

Appendix E) Maximum Cable Lengths

Cable	Maximum Length
Ethernet	100 metres
ISDN S/T	10 metres
Telephone cable	152 metres